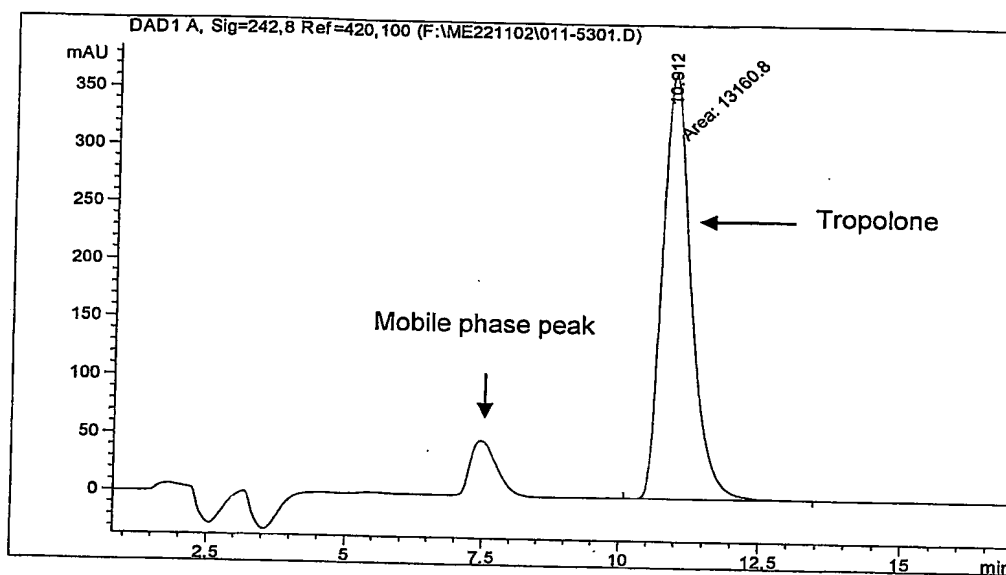
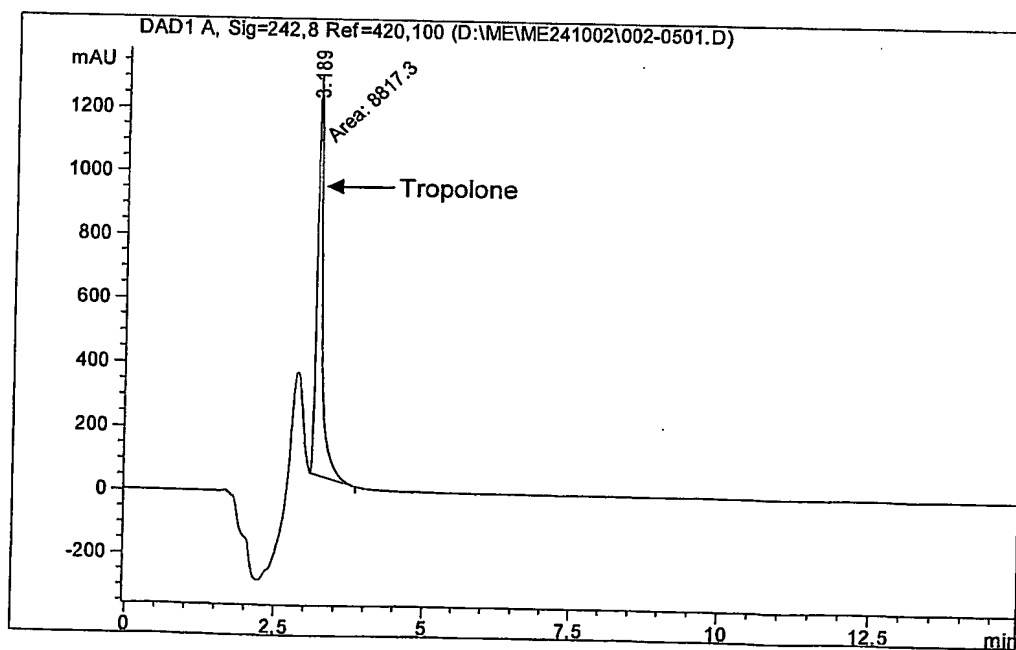


**Figure 1a:** Tropolone Standard (2.0  $\mu\text{g/mL}$ ) Analysed on an ACE C18 2.1 mm RP HPLC column in a 0.1%  $\text{CuSO}_4$ / 0.3% HSA / 10% Acetonitrile Mobile Phase. Top Panel: Tropolone Standard.

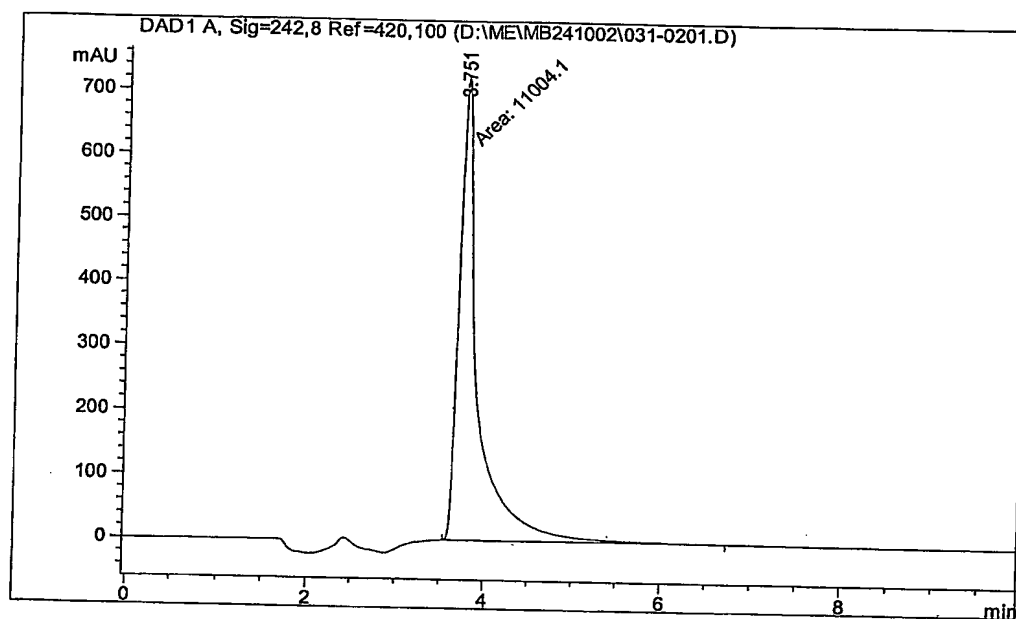


**Figure 1b:** Tropolone Standard (2.0  $\mu\text{g/mL}$ ) Analysed on an ACE C18 2.1 mm RP HPLC Column Using a 0.1%  $\text{CuSO}_4$ / 0.1% TFA / 10% Acetonitrile Mobile Phase




2/6

**Figure 1c: Tropolone Standard ( 2.0 µg/mL) Analysed on an ACE C18 2.1 mm RP HPLC Column Using a 0.1% CuSO<sub>4</sub>/ 0.1% MSA / 10% Acetonitrile Mobile Phase**




**Figure 1d:** Tropolone Standard (0.1 µg/mL) Analysed on an ACE C18 2.1 mm RP HPLC Column in a 0.1% CuSO<sub>4</sub>/ 0.3% HSA / 10% Acetonitrile Mobile Phase. Top Panel: Tropolone Standard, Bottom Panel: Mobile Phase

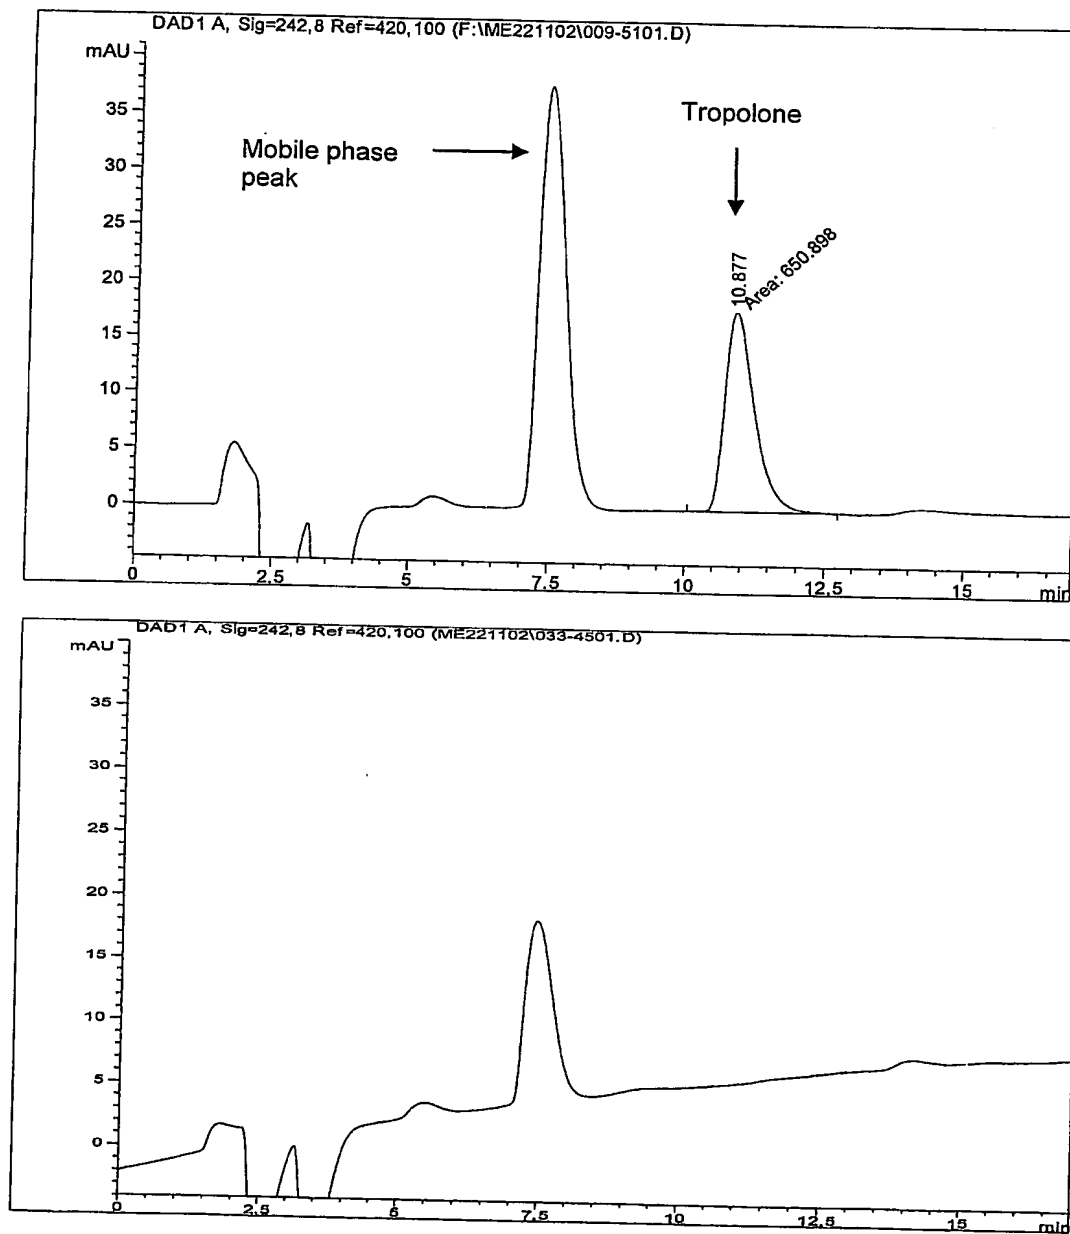


4/6

**Figure 2a: Example Chromatograms of Non-Spiked Lot 11859 and Buffer Control.**

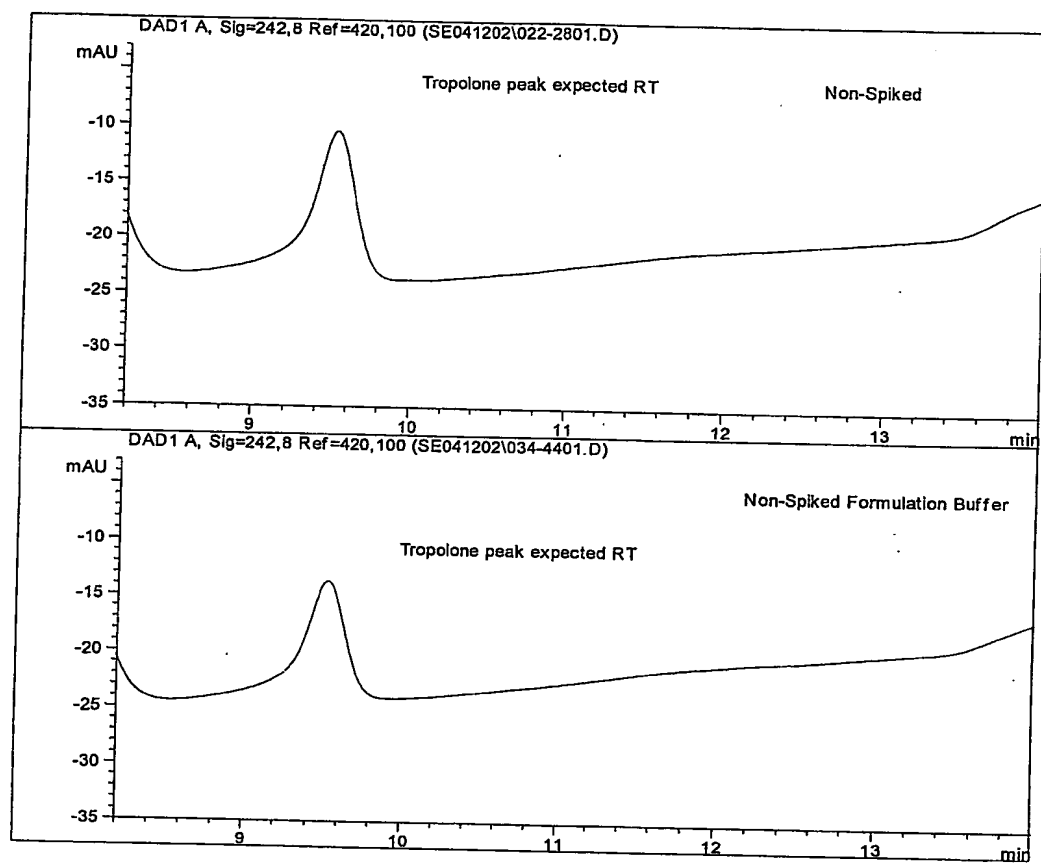

5/6

**Figure 2b: Example Chromatograms of Tropolone Spiked (10 ng/mL)  
Lot 11859 and Buffer**

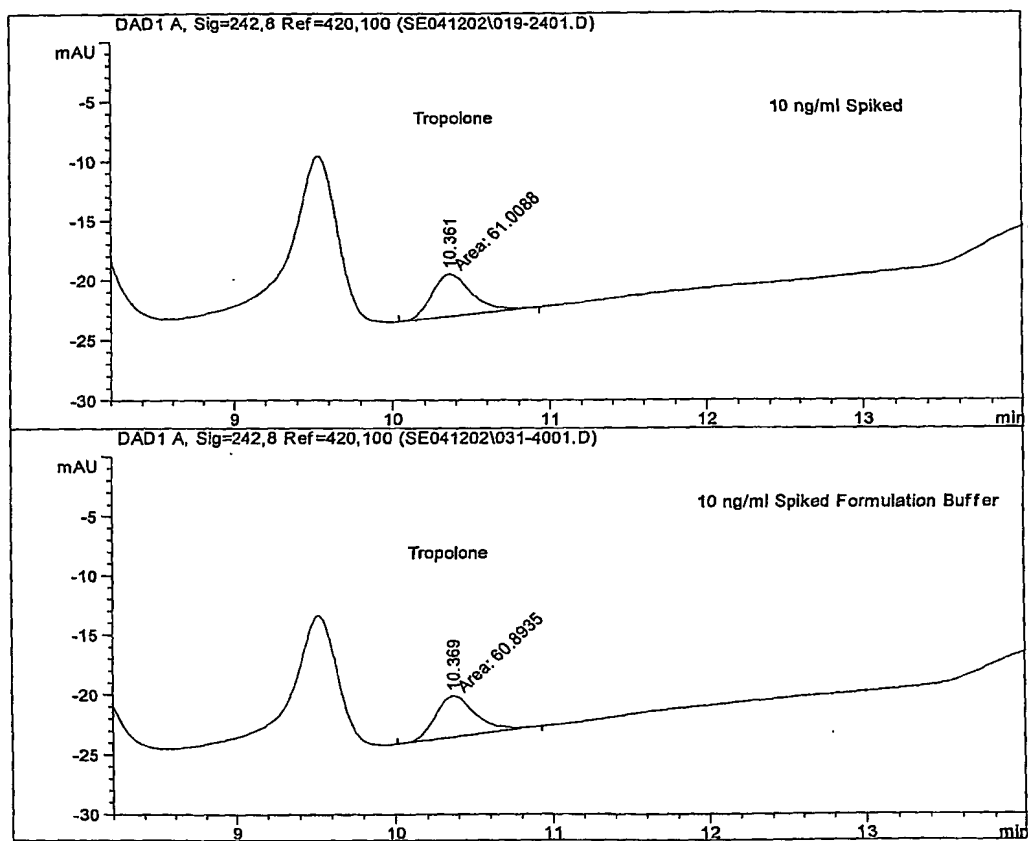

6/6

**Figure 2c: Example Chromatograms of 100 ng/mL Tropolone Spiked Lot 11859 and Buffer**

